


CO₂ LASERS

Air & Water-Cooled

ULR-50

FEATURES

- Air and water-cooled options
- Class IV configurations available
- Integrated RF supply
- New TTL output temperature warning LED
- New fault indicator LED
- New lowprofile mounting plate
- Excellent power stability
- Quiet operation
- Manufactured with proven ULS technology

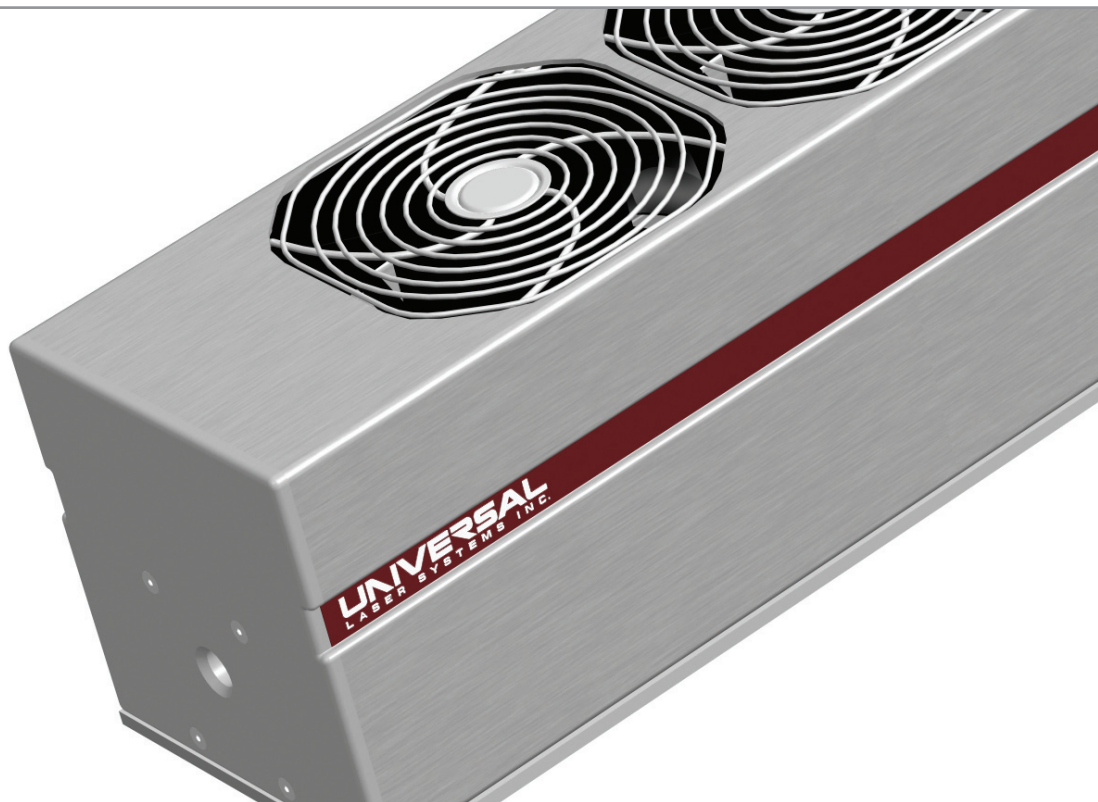

LASER SPECIFICATIONS*


Rated Power**	50 W
Wavelength	10.6 μ
Power Stability	$\pm 5\%$ after 15 minutes of CW operation
M ²	1.4 \pm 0.2
Beam Size (Near Field) [†]	4 \pm 1mm
Beam Divergence (Full Angle)	5 \pm 1mR
Polarization	Linear
Pointing Stability	200 μ R
Optical Pulse Rise or Fall Time	120 \pm 40 μ S
Optical Delay Time	38 \pm 10 μ S
Optical Modulation	100% up to 5KHz
Modulation Signal Type	TTL Compatible

LASER SPECIFICATIONS*


Cooling	Integrated Air/Water
Weight (Air-cooled)	28 lbs (12.7 kg) - Class IV
	21 lbs (9.5 kg) - OEM
Dimensions	see rear panel
<i>Environmental</i>	
Ambient Temperature ^{††}	50-95°F (10-35°C)
Relative Humidity	<90% (non-condensing)
<i>Power Requirements</i>	
DC Input Voltage	48 VDC
RMS Current (CW, with fan)	20 A

*These specifications are subject to change without notice. **Output power is guaranteed to exceed this level for a period of 15 months from date of purchase, regardless of use. [†]Near field approximately 150mm from output coupler. ^{††}At temperatures below 50°F [10°C] operation may be intermittent and there is a potential for damage to the power supply and optics.

≡ BASIC CONFIGURATION (WATER-COOLED SHOWN BELOW)

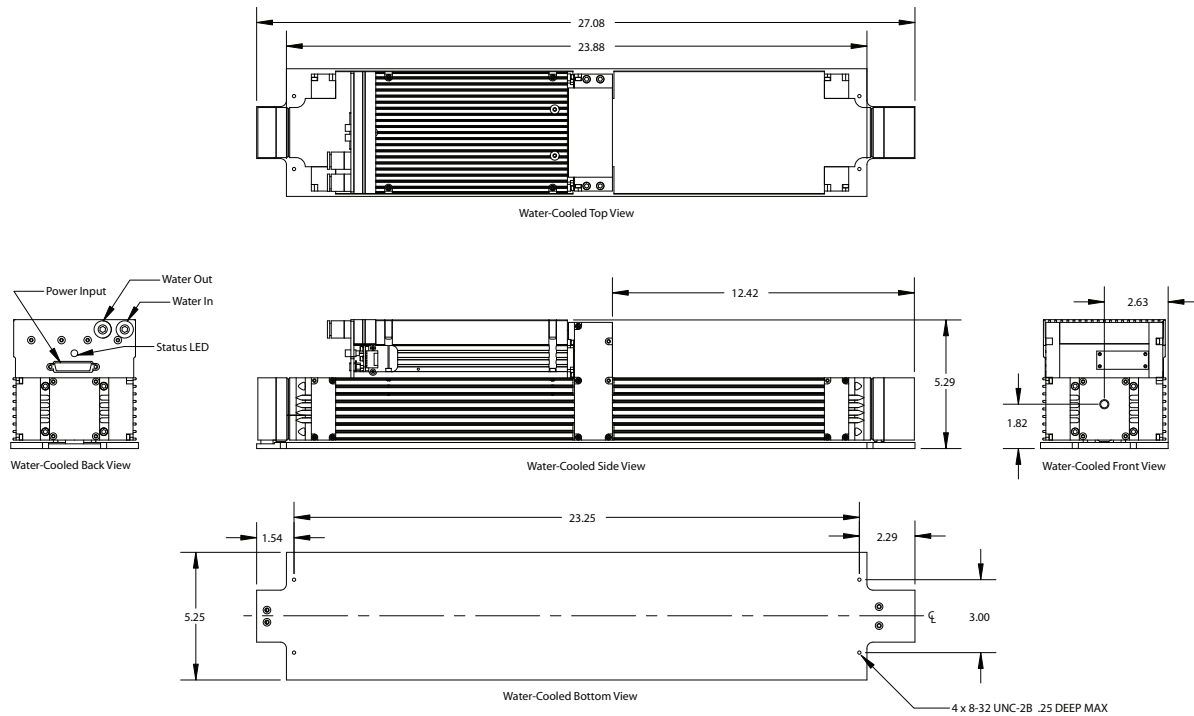

≡ INTEGRATED COOLING/CLASS IV CONFIGURATIONS (CLASS IV AIR-COOLED SHOWN BELOW)

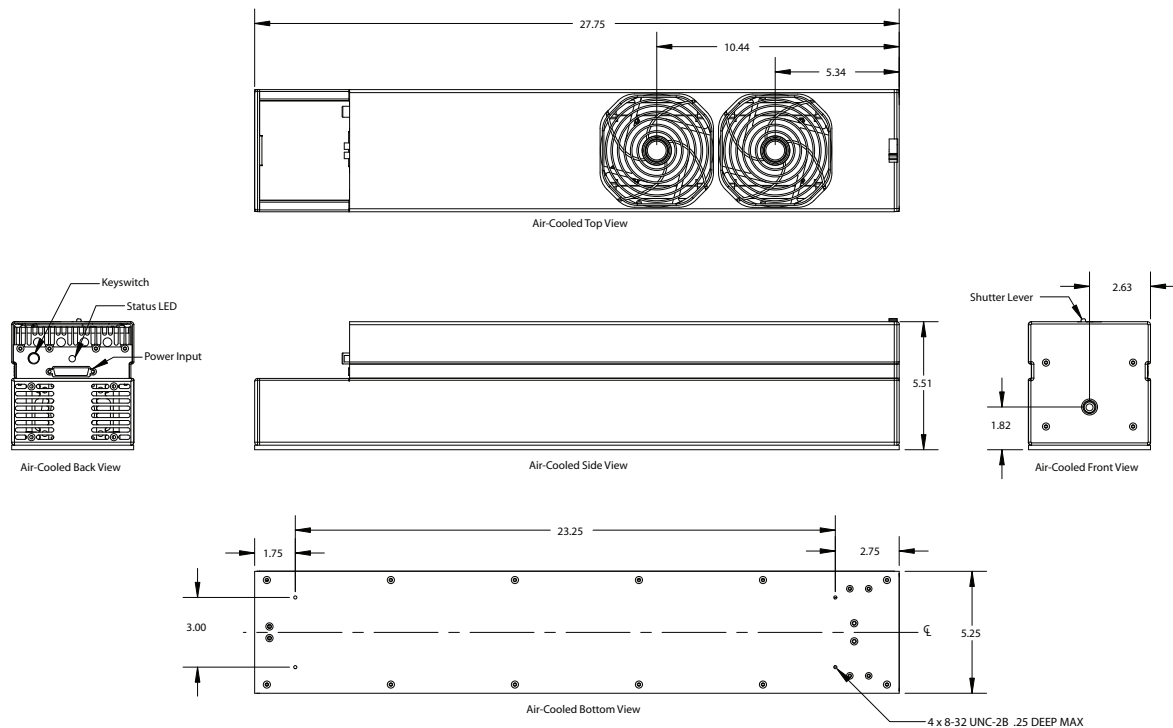

These OEM lasers are components intended for integration into OEM equipment and as such do not comply with the Federal regulations (21 CFR Subchapter J) as administered by the Center for Devices and Radiological Health. Purchaser acknowledges that it is his responsibility to obtain compliance with all CDRH and other applicable domestic and/or international safety standards. Protected under U.S. patents 5,661,746; 5,754,575; 5,867,517; 5,901,167; 5,894,493; 5,881,087; 5,982,803; 6,181,719; 6,983,001; 7,060,934; D517,474. Other U.S. and international patents pending. ©2006 Universal Laser Systems, Inc.

WARNING: UNIVERSAL LASER SYSTEMS PRODUCTS ARE NOT DESIGNED, TESTED, INTENDED OR AUTHORIZED FOR USE IN ANY MEDICAL APPLICATIONS, SURGICAL APPLICATIONS, MEDICAL DEVICE MANUFACTURING, OR ANY SIMILAR PROCEDURE OR PROCESS REQUIRING APPROVAL, TESTING, OR CERTIFICATION BY THE UNITED STATES FOOD AND DRUG ADMINISTRATION OR OTHER SIMILAR GOVERNMENTAL ENTITIES. SHOULD THE BUYER USE UNIVERSAL LASER SYSTEMS PRODUCTS FOR ANY SUCH UNINTENDED OR UNAUTHORIZED APPLICATION, ALL WARRANTIES REGARDING THE UNIVERSAL LASER SYSTEMS PRODUCTS SHALL BE NULL AND VOID. FURTHER, THE BUYER SHALL HAVE NO REMEDY AGAINST UNIVERSAL LASER SYSTEMS AND ITS OFFICERS, EMPLOYEES, SUBSIDIARIES, AFFILIATES AND DISTRIBUTORS FOR, AND THE BUYER SHALL INDEMNIFY AND HOLD THOSE PARTIES HARMLESS AGAINST, ANY AND ALL CLAIMS, COSTS, DAMAGES, EXPENSES AND REASONABLE ATTORNEY FEES ARISING OUT OF, DIRECTLY OR INDIRECTLY, ANY CLAIM ASSOCIATED WITH SUCH UNINTENDED OR UNAUTHORIZED USE, INCLUDING BUT NOT LIMITED TO ANY CLAIM BASED ON WARRANTY (EXPRESS OR IMPLIED), CONTRACT, TORT (INCLUDING ACTIVE, PASSIVE, OR IMPUTED NEGLIGENCE), STRICT LIABILITY, PATENT OR COPYRIGHT INFRINGEMENT OR MISAPPROPRIATION OF INTELLECTUAL PROPERTY.